

# OPERATING INSTRUCTIONS



Translation of the original instructions

## PTR 91

FullRange® Gauge


BG-5041 BEN/B (2016-07)





**PFEIFFER**  **VACUUM**



## Product Identification

In all communications with Pfeiffer Vacuum, please specify the information given on the product nameplate. For convenient reference copy that information into the space provided below.



Pfeiffer Vacuum, D-35614 Asslar			
Typ:.....			
No:.....			
F-Nc:.....			
.....VDC .....	.....W	3103457	

## Validity

This document applies to products with part numbers:

- |                |                |
|----------------|----------------|
| PT T03 148 310 | (DN 25 ISO-KF) |
| PT T03 158 310 | (DN 40 ISO-KF) |
| PT T03 358 310 | (DN 40 CF-F)   |

The part number (No) can be taken from the product nameplate.

If not indicated otherwise in the legends, the illustrations in this document correspond to gauges with vacuum connection DN 25 ISO-KF. They apply to the other gauges by analogy.

We reserve the right to make technical changes without prior notice.



## Intended Use

The FullRange® Gauges PTR 91 have been designed for vacuum measurement of gases in the pressure range of  $1 \times 10^{-9}$  ... 1000 mbar.

They must not be used for measuring flammable or combustible gases in mixtures containing oxidants (e.g. atmospheric oxygen) within the explosion range.

They are intended for operation in connection with a Pfeiffer Vacuum measurement unit for gauges or with another suitable controller.

## Functional Principle

The gauge consists of two separate measuring systems (the Pirani and the cold cathode system according to the inverted magnetron principle). They are combined in such a way that for the user, they behave like one measuring system.

Over the whole measurement range, the measuring signal is output as a logarithm of the pressure.

## Scope of Delivery

- 1× gauge
- 1× pin for adjusting settings via buttons
- 1× Operating Instructions German
- 1× Operating Instructions English

## Trademark

FullRange® Pfeiffer Vacuum GmbH




## Contents

Product Identification	2
Validity	2
Intended Use	3
Functional Principle	3
Scope of Delivery	3
Trademark	3
<b>1 Safety</b>	<b>6</b>
1.1 Symbols Used	6
1.2 Personnel Qualifications	6
1.3 General Safety Instructions	7
1.4 Liability and Warranty	7
<b>2 Technische Daten</b>	<b>8</b>
2.1 Output Signal vs. Pressure	12
2.2 Gas Type Dependence PTR 91	13
<b>3 Installation</b>	<b>16</b>
3.1 Vacuum Connection	16
3.2 Power Connection	20
<b>4 Operation</b>	<b>22</b>
4.1 Status Indication	22
4.2 Put Gauge Into Operation	23
4.3 Gas Type Dependence	23
4.4 Ignition Delay	24
4.7 Contamination	24
<b>5 Deinstallation</b>	<b>26</b>
<b>6 Maintenance, Repair</b>	<b>28</b>
6.1 Adjusting the Gauge	28
6.2 Cleaning the Gauge / Replacing Parts	30
6.2.1 Troubleshooting (measuring chamber)	31
6.2.2 Replacing Ionization Chamber and Ignition Aid	33
6.2.3 Replacing Measuring Chamber	35
6.3 Troubleshooting	37
<b>7 Returning the Product</b>	<b>39</b>



<b>8 Disposal</b>	<b>40</b>
<b>9 Options</b>	<b>41</b>
<b>10 Accessories</b>	<b>41</b>
<b>11 Spare Parts</b>	<b>42</b>
11.1 Ignition Aid	42
11.2 Ionization chamber	42
11.3 Measuring Chamber Cpl. (Spare Sensor)	43
<b>ETL Certification</b>	<b>44</b>
<b>EU Declaration of Conformity</b>	<b>45</b>

For cross-references within this document, the symbol (→  XY) is used.



# 1 Safety

## 1.1 Symbols Used

**DANGER**

Information on preventing any kind of physical injury.

**WARNING**

Information on preventing extensive equipment and environmental damage.

**Caution**

Information on correct handling or use. Disregard can lead to malfunctions or minor equipment damage.



Consultation of operating manual required (symbol printed on the product nameplate)



Notice



Labeling

## 1.2 Personnel Qualifications

**Skilled personnel**

All work described in this document may only be carried out by persons who have suitable technical training and the necessary experience or who have been instructed by the end-user of the product.



### 1.3 General Safety Instructions

- Adhere to the applicable regulations and take the necessary precautions for the process media used.  
Consider possible reactions with the product materials.  
Consider possible reactions (e.g. explosion) of the process media due to the heat generated by the product.
- Adhere to the applicable regulations and take the necessary precautions for all work you are going to do and consider the safety instructions in this document.
- Before beginning to work, find out whether any vacuum components are contaminated. Adhere to the relevant regulations and take the necessary precautions when handling contaminated parts.

Communicate the safety instructions to all other users.

### 1.4 Liability and Warranty

Pfeiffer Vacuum assumes no liability and the warranty becomes null and void if the end-user or third parties


- disregard the information in this document
- use the product in a non-conforming manner
- make any kind of interventions (modifications, alterations etc.) on the product
- use the product with accessories not listed in the product documentation.

The end-user assumes the responsibility in conjunction with the process media used.

Gauge failures due to contamination or wear and tear, as well as expendable parts (e.g. ionization chamber, ignition aid, Pirani filament), are not covered by the warranty.




## 2 Technical Data


Measurement range (air, N <sub>2</sub> )	1×10 <sup>-9</sup> ... 1000 mbar
Accuracy (N <sub>2</sub> )	
1×10 <sup>-8</sup> ... 100 mbar	30% of reading
100 ... 1000 mbar	50% of reading
Repeatability (N <sub>2</sub> )	
1×10 <sup>-8</sup> ... 100 mbar	5% of reading
Gas type dependence	→  13
Voltage range (analog output)	0 ... +10.5 V
Measurement range	+1.397 ... +8.6 V (dc)
Voltage vs. pressure	0.6 V/decade, logarithmic
Error signal	+9.5 ... +10.5 V (dc)
Output impedance	2 × 4.7 Ω, short-circuit proof
Load impedance	≥10 kΩ, short-circuit proof
Step response time	pressure dependent
>1×10 <sup>-6</sup> mbar	<100 ms
1×10 <sup>-6</sup> ... 1×10 <sup>-8</sup> mbar	≈1 s
Gauge identification	85 kΩ referenced to supply common
Status signal (digital output)	
Current rating	100 mA
High voltage is ON	+14.5 ... +30 V (dc) (depending on supply voltage)
High voltage is OFF	0 V (dc)





## Supply


**DANGER**



The gauge may only be connected to power supplies, instruments, or control devices that conform to the requirements of a grounded protective extra-low voltage (PELV) and limited power source (LPS), Class 2. The connection to the gauge has to be fused. <sup>1)</sup>

Supply voltage at the gauge <sup>2)</sup>	Class 2 / LPS +14.5 ... +30 V (dc)
Ripple	$\leq 1 V_{pp}$
Power consumption	$\leq 2 W$
Fuse to be connected <sup>1)</sup>	$\leq 1 AT$
<hr/>	
High voltage in the measuring chamber	
Ignition voltage	$\leq 4.5 kV$
Operating voltage	$\leq 3.3 kV$
Current in the measuring chamber	
	High current
<hr/>	
Electrical connection	FCC 68, 8-pin
Sensor cable	8-pin, shielded
Cable length	$\leq 50 m (0.14 mm^2/conductor)$
Grounding concept	
	→ "Power Connection"
Vacuum connection – signal common	connected via 10 k $\Omega$ (potential difference $\leq 16 V$ )
Supply common – signal common	conducted separately; differential measurement is recommended

<sup>1)</sup> Pfeiffer Vacuum controllers fulfill this requirement.

<sup>2)</sup> The minimum voltage of the power supply unit must be increased proportionally to the length of the sensor cable.



<b>Materials exposed to vacuum</b>	
Vacuum connection	stainless steel (1.4435)
Measuring chamber	stainless steel (1.4435)
Pirani filament	W
<b>Feedthrough</b>	
Isolation	glass, ceramic (Al <sub>2</sub> O <sub>3</sub> )
Ring	stainless steel (1.4435)
Anode	molybdenum
Pin	Ni alloy
Ionization chamber	stainless steel (1.4301, 1.4016)
Ignition aid	stainless steel (1.4310)
<b>Internal volume</b>	
DN 25 ISO-KF	≈19.9 cm <sup>3</sup>
DN 40 ISO-KF	≈20.9 cm <sup>3</sup>
DN 40 CF-F	≈25.2 cm <sup>3</sup>
Permissible pressure (absolute)	10 bar, limited to inert gases <55 °C
Bursting pressure (absolute)	>13 bar
<hr/>	
<b>Permissible temperatures</b>	
Operation	+5 °C ... +55 °C
Pirani filament (PTR 91)	120 °C
Bakeout	≤150 °C <sup>3)</sup>
Storage	-40 °C ... +70 °C
<b>Relative humidity for 30 days a year</b>	
1×10 <sup>-8</sup> ... 1×10 <sup>-2</sup> mbar	≤70% (non-condensing)
1×10 <sup>-7</sup> ... 1×10 <sup>-2</sup> mbar	≤95% (non-condensing)
Mounting orientation	any
Use	indoors only, altitude up to 6000 m NN
Degree of protection	IP 40
<hr/>	



<sup>3)</sup> Without electronics unit.




## Dimensions [mm]



DN 25 ISO-KF



DN 40 ISO-KF



DN 40 CF-F


## Weight

DN 25 ISO-KF	<280 g
DN 40 ISO-KF	<320 g
DN 40 CF-F	<570 g



## 2.1 Output Signal vs. Pressure

Pressure p

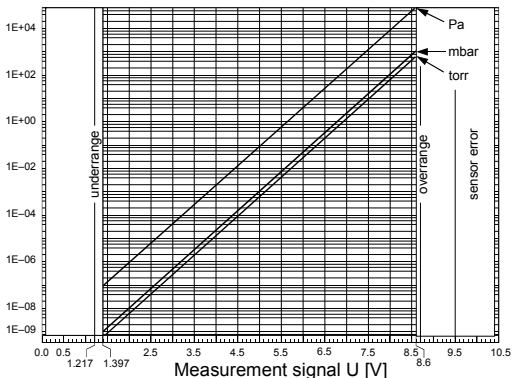

$$p = 10^{1.667U-d} \quad \Leftrightarrow \quad U = c + 0.6 \log p$$

valid in the range  $1 \times 10^{-9} \text{ mbar} < p < 1000 \text{ mbar}$   
 $7.5 \times 10^{-10} \text{ Torr} < p < 750 \text{ Torr}$   
 $1 \times 10^{-7} \text{ Pa} < p < 1 \times 10^5 \text{ Pa}$

	mbar	Pa	Torr
c	6.798	5.598	6.873
d	11.33	9.333	11.46


where p pressure  
 U measurement signal  
 c, d constant (pressure unit dependent)



## 2.2 Gas Type Dependence PTR 91


### Indication range from $10^2 \dots 10^{-2}$ mbar (Pirani-only operation)

Indicated pressure (gauge calibrated for air)

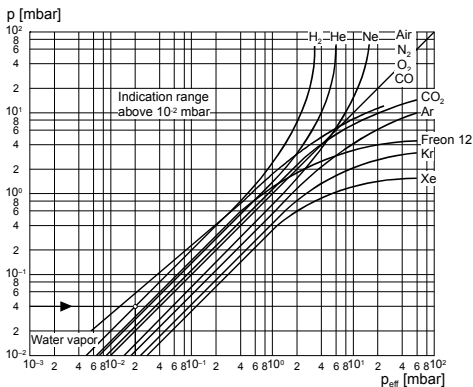

## Indication range $10^{-6} \dots 0.1$ mbar

Indicated pressure (gauge calibrated for air)

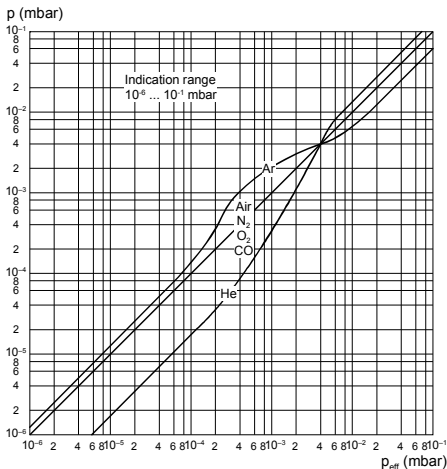

## Indication range below $10^{-5}$ mbar

In the range below  $10^{-5}$  the pressure indication is linear. For gases other than air, the pressure can be determined by means of a simple conversion formula:

$$p_{\text{eff}} = K \times \text{indicated pressure}$$



where:	Gas type	K
	Air (N <sub>2</sub> , O <sub>2</sub> , CO)	1.0
	Xe	0.4
	Kr	0.5
	Ar	0.8
	H <sub>2</sub>	2.4
	Ne	4.1
	He	5.9

These conversion factors are average values.



A mixture of gases and vapors is often involved. In this case, accurate determination is only possible with a partial pressure measurement instrument, e.g. a quadrupole mass spectrometer.



## 3 Installation

### 3.1 Vacuum Connection



**DANGER**

**DANGER:** overpressure in the vacuum system  
>1 bar

Injury caused by released parts and harm caused by escaping process gases can result if clamps are opened while the vacuum system is pressurized.

Do not open any clamps while the vacuum system is pressurized. Use the type clamps which are suited to overpressure.



**DANGER**

**DANGER:** overpressure in the vacuum system  
>2.5 bar

KF flange connections with elastomer seals (e.g. O-rings) cannot withstand such pressures. Process media can thus leak and possibly damage your health.

Use O-rings provided with an outer centering ring.





**DANGER**

**DANGER:** protective ground

Products that are not correctly connected to ground can be extremely hazardous in the event of a fault.

Electrically connect the gauge to the grounded vacuum chamber. This connection must conform to the requirements of a protective connection according to EN 61010:

- CF connections fulfill this requirement
- For gauges with a KF flange, use a conductive metallic clamping ring.

**Caution**

**Caution:** vacuum component

Dirt and damages impair the function of the vacuum component.

When handling vacuum components, take appropriate measures to ensure cleanliness and prevent damages.

**Caution**

**Caution:** dirt sensitive area


Touching the product or parts thereof with bare hands increases the desorption rate.

Always wear clean, lint-free gloves and use clean tools when working in this area.




Mount the gauge so that no vibrations occur. Vibrations at the gauge cause a deviation of the measured values.

The gauge may be mounted in any orientation. To keep condensates and particles from getting into the measuring chamber preferably choose a horizontal to upright position.

For potentially contaminating applications and to protect the measurement system against contamination, installation of the optional seal with centering ring and filter is recommended (Options →  41).

Remove the protective lid and connect the product to the vacuum system.

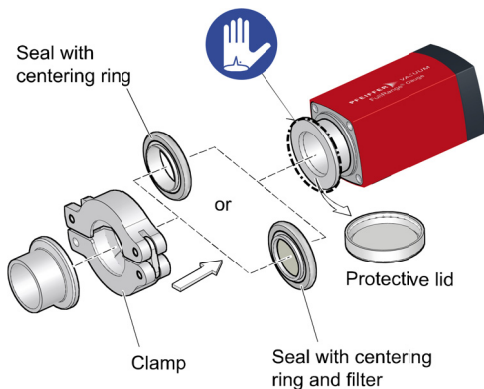


Keep the protective lid.





When making a CF flange connection, it may be advantageous to temporarily remove the electronics unit.

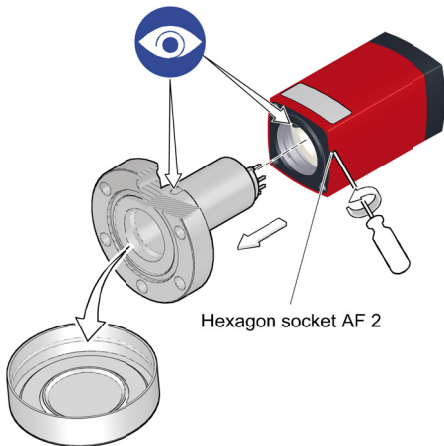

Hexagon socket AF 2

Protective lid



Keep the protective lid.



**WARNING**



WARNING: electric arcing


Helium may cause electric arcing with detrimental effects on the electronics of the product.

Before performing any tightness tests put the product out of operation and remove the electronics unit.



## 3.2 Power Connection



Make sure the vacuum connection is properly made  
(→  16).



### DANGER

The gauge may only be connected to power supplies, instruments or control devices that conform to the requirements of a grounded protective extra-low voltage (PELV) and limited power source (LPS), Class 2. The connection to the gauge has to be fused. <sup>4)</sup>




Ground loops, differences of potential, or EMC problems may affect the measurement signal. For optimum signal quality, please do observe the following notes:

- Use an overall metal braided shielded cable. The connector must have a metal case.
- Connect the supply common with protective ground directly at the power.
- Use differential measurement input (signal common and supply common conducted separately).
- Potential difference between supply common and housing  $\leq 18$  V (overvoltage protection).

<sup>4)</sup> Pfeiffer Vacuum controllers fulfill these requirements.




If no sensor cable is available, make one according to the following diagram. Connect the sensor cable.

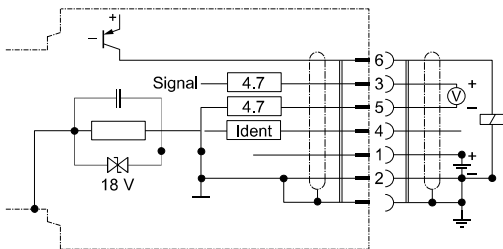

### Electrical connection

- Pin 1 Supply (14.5 ... 30 V (dc))
- Pin 2 Supply common GND
- Pin 3 Signal output (measuring signal)
- Pin 4 Gauge identification
- Pin 5 Signal common
- Pin 6 Status signal




Pin 7 and 8 are not assigned.

FCC 68  
8-pin



## 4 Operation

### 4.1 Status Indication

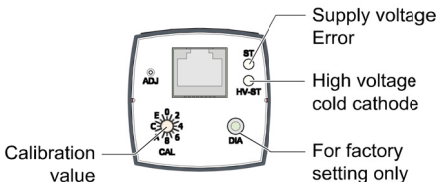


LED		Meaning
<ST>	<HV-ST>	
off	off	No supply voltage
lit solid green	off	Supply voltage = ok, no high voltage in the measuring chamber
lit solid yellow	blinking green	Supply voltage = ok, pressure in the cold cathode range, cold cathode has not ignited
lit solid green	lit solid green	Cold cathode has ignited
blinking red	off	EEPROM error
lit solid yellow	lit solid green	Over- or underrange

Troubleshooting (→ 38).



## 4.2 Put Gauge Into Operation


When the supply voltage is applied, the measuring signal is available at the signal output (→  20).

Allow for a stabilizing time of approx. 10 min. Once the gauge has been switched on, it can remain in operation permanently irrespective of the pressure.

### Measurement Principle, Measuring Behavior

The gauge consists of two separate measuring systems (Pirani and cold cathode system according to the inverted magnetron principle). They are combined in such a way that for the user, they behave like one measuring system.


The optimum measuring configuration for the particular pressure range, in which measurement is performed, is used:




- The Pirani measuring circuit is always on
- The cold cathode measuring circuit is controlled by the Pirani circuit and is activated only at pressures  $p < 1 \times 10^{-2}$  mbar

As long as the cold cathode measuring circuit has not ignited, the measuring value of the Pirani is output as measuring signal (if  $p < 5 \times 10^{-4}$  mbar: "Pirani-Underrange" is displayed).

## 4.3 Gas Type Dependence

The measurement value is gas dependent. The pressure reading applies to dry air, O<sub>2</sub>, CO and N<sub>2</sub>. For other gases, it has to be corrected (→  13).

If the gauge is operated with a Pfeiffer Vacuum controller, a calibration factor for correction of the actual reading can be applied (→  of the corresponding controller).



## 4.4 Ignition Delay

An ignition delay occurs when cold cathode gauges are switched on. The delay time increases at low pressures and for clean, degassed gauges it is typically:

$1 \times 10^{-5} \dots 1 \times 10^{-2}$ mbar	< 1	second
$1 \times 10^{-7} \dots 1 \times 10^{-5}$ mbar	< 20	seconds
$5 \times 10^{-9} \dots 1 \times 10^{-7}$ mbar	< 2	minutes
$< 5 \times 10^{-9}$ mbar	< 20	minutes

The ignition is a statistical process. Already a small amount of depositions on the inner surfaces can have a strong influence on it.

As long as the cold cathode measuring circuit has not ignited, the measuring value of the Pirani is output as measuring signal ("Pirani-Underrange" is displayed for pressures  $p < 5 \times 10^{-4}$  mbar). The identification output (pin 1) indicates the Pirani-only operation.



If the gauge is activated at a pressure  $p < 3 \times 10^{-9}$  mbar, the gauge cannot recognize whether the cold cathode system has ignited. It indicates "Pirani-Underrange".



Once flanged on, permanently leave the gauge in the operating mode irrespective of the pressure range. Like this, the ignition delay of the cold cathode measuring circuit is always negligible (<1 s), and thermal stabilizing effects are minimized.

## 4.5 Contamination


Gauge failures due to contamination or wear and tear, as well as expendable parts (e.g. ionization chamber, ignition aid, Pirani filament), are not covered by the warranty.





Gauge contamination is influenced by the process media used as well as any existing or new contaminants and their respective partial pressures. Continuous operation in the range of  $10^{-4}$  mbar ...  $10^{-2}$  mbar can cause severe contamination as well as reduced up-time.

Contamination of the gauge generally causes a deviation of the measured values:

- In the high pressure range ( $1 \times 10^{-3}$  mbar ... 0.1 mbar), the pressure reading is too high (contamination of the Pirani element). Readjustment of the Pirani →  28.
- In the low pressure range ( $p < 1 \times 10^{-3}$  mbar), the pressure indication is usually too low (as a consequence of the contamination of the cold cathode system). In case of severe contamination, instabilities can occur (layers of the measuring chamber peel off). Contamination due to isolating layers can even lead to a complete failure of the discharge ("Underrange" is displayed).

Contamination can to a certain extent be reduced by:

- geometric protection (e.g. screenings, elbows) against particles that spread rectilinearly
- mounting the flange of the gauge at a place where the partial pressure of the pollutants is particularly low.

Special precautions are required for vapors deposited under plasma (of the cold cathode measuring system). While vapors occur it may even be necessary

- to temporarily switch of the gauge
- to temporarily seal off of the gauge from the vacuum chamber using a valve.



## 5 Deinstallation

 **DANGER**

**DANGER:** contaminated parts

Contaminated parts can be detrimental to health and environment.

Before beginning to work, find out whether any parts are contaminated. Adhere to the relevant regulations and take the necessary precautions when handling contaminated parts.

**Caution**

**Caution:** vacuum component

Dirt and damages impair the function of the vacuum component.

When handling vacuum components, take appropriate measures to ensure cleanliness and prevent damages.

**Caution**

**Caution:** dirt sensitive area

Touching the product or parts thereof with bare hands increases the desorption rate.

Always wear clean, lint-free gloves and use clean tools when working in this area.


- 1** Vent the vacuum system.
- 2** Put the gauge out of operation and disconnect the sensor cable.



- 3** Remove gauge from the vacuum system and install the protective lid.



When deinstalling the CF flange connection, it may be advantageous to temporarily remove the electronics unit (→ 19).

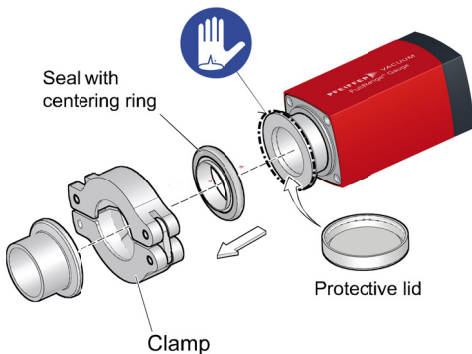

## 6 Maintenance, Repair



Gauge failures due to contamination and wear and tear, as well as expendable parts (e.g. ionization chamber, ignition aid, Pirani filament), are not covered by the warranty.

Pfeiffer Vacuum assumes no liability and the warranty becomes null and void if any repair work is carried out by the end-user or third parties.

### 6.1 Adjusting the Gauge

The cold cathode measuring circuit, which is dominant for low pressures ( $<1 \times 10^{-3}$  mbar), is factory-calibrated and cannot be adjusted. The HV adjustment of the Pirani measuring circuit is carried out automatically by the gauge itself at pressures  $<1 \times 10^{-5}$  mbar. The new zero point is saved non-volatile every 15 minutes. Any adjustment has a negligible effect on the pressure range between approx.  $10^{-2}$  mbar and  $10^2$  mbar.

If used under different climatic conditions, through extreme temperatures, aging or contamination the characteristic curve can be offset and a manually readjustment or a maintenance may become necessary.

An adjustment via the <ADJ> button can become necessary (procedure → ❶, ❷), if pressure values  $<10^{-2}$  mbar are no longer output.


For adjusting the zero, operate the gauge under the same constant ambient conditions and in the same mounting orientation as normally.



If you are using a seal with centering ring and filter, check that they are clean or replace them if necessary (→ "Deinstallation").



- Put the gauge into operation and operate it at atmospheric pressure for at least 10 minutes.
- Press the <ADJ> button with a pin (max.  $\varnothing 1.1$  mm) and the ATM adjustment is carried out: The Pirani sensor is adjusted to 1000 mbar (duration  $\approx 5$  s).




- ✓ If the pressure value 1000 mbar is output at the measurement value output, the adjustment has been successful. Otherwise, repeat the adjustment procedure.
- Evacuate the vacuum system to  $p < 10^{-5}$  mbar and wait at least 2 minutes.
  - Press the <ADJ> button with a pin and the HV adjustment is carried out (duration  $\approx 5$  s).
- ✓ If the pressure value  $1 \times 10^{-5}$  mbar is output at the measurement value output, the adjustment has been successful. Otherwise, repeat the adjustment procedure.



## 6.2 Cleaning the Gauge / Replacing Parts



In case of severe contamination or defective (e.g. Pirani filament rupture), replace the complete measuring chamber (Spare Parts →  42).



### DANGER



**DANGER:** contaminated parts

Contaminated parts can be detrimental to health and environment.

Before beginning to work, find out whether any parts are contaminated. Adhere to the relevant regulations and take the necessary precautions when handling contaminated parts.



### Caution



**Caution:** vacuum component

Dirt and damages impair the function of the vacuum component.

When handling vacuum components, take appropriate measures to ensure cleanliness and prevent damages.



### Caution






**Caution:** dirt sensitive area

Touching the product or parts thereof with bare hands increases the desorption rate.

Always wear clean, lint-free gloves and use clean tools when working in this area.



	 <b>DANGER</b>
	<p><b>DANGER:</b> cleaning agents</p> <p>Cleaning agents can be detrimental to health and environment.</p> <p>Adhere to the relevant regulations and take the necessary precautions when handling and disposing of cleaning agents. Consider possible reactions with the product materials (→  10).</p>

### Precondition

Gauge deinstalled.


## 6.2.1 Troubleshooting (measuring chamber)



If the cause of the fault is suspected to be in the measuring chamber, the following checks can be made with an ohmmeter.

### Tools / material required

- Allen wrench AF 2
- Pliers for retaining ring
- Ohmmeter

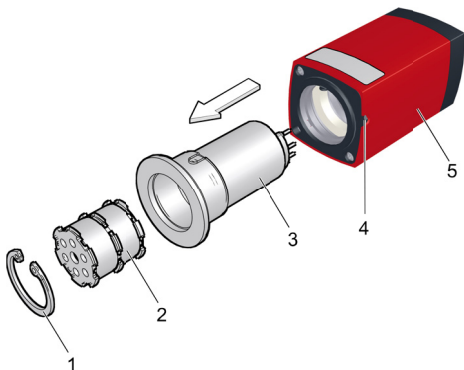






- 1** Unfasten the hexagon socket set screw (4) and remove the complete measuring chamber (3) from the electronics unit (5).
- 2** Remove the retaining ring (1) as well as the ionization chamber (2) from the measuring chamber (3).
- 3** Check the ionization chamber and the measuring chamber for contamination:
  - Ionization chamber is contaminated only: Replace ionization chamber (→  33)
  - Measuring chamber is severely contaminated: Replace complete measuring chamber (→  35).






- 4** Using an ohmmeter, make following measurements on the contact pins.

Measurement between pins			Possible cause
1 + 4	39.5 ... 40.5 $\Omega$ (at 20 °C)	Values outside of the range	Pirani filament rupture
1 + 2	1000 ... 1100 $\Omega$ (at 20 °C)	Values outside of the range	Pirani temperature sensor rupture
5 + measuring chamber	$\infty$	$\ll \infty$	Contamination, short circuit cold cathode

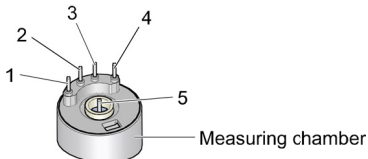



All of these faults can only be remedied by replacing the complete measuring chamber (→  35).

- 5** We recommend to perform a leak test (leak rate  $<1 \times 10^{-9}$  mbar l/s).

## 6.2.2 Replacing Ionization Chamber and Ignition Aid

### Precondition

Troubleshooting (measuring chamber) performed (→  31).


- 1** Due to contamination remove the ignition aid with the removing tool (Accessories →  41).




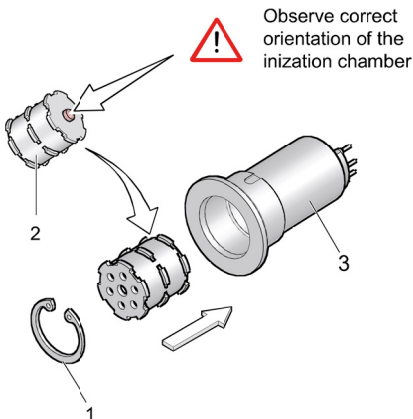
- 2** We recommend to rub the inside walls of the measuring chamber up to the groove for the retaining ring to a bright finish using a polishing cloth.



- The sealing surfaces must only be worked concentrically.
- Do not bend the anode.

- 3** Insert the new ignition aid into the mounting tool and slide it onto the anode (Spare Parts →  42).

- 4** Slide a new ionization chamber (2) into the measuring chamber (3) until the mechanical stop is reached and mount the retaining ring (1) (Spare Parts →  42).





- 5** We recommend to perform a leak test (leak rate  $<1 \times 10^{-9}$  mbar l/s).



- ⑥ Carefully slide the measuring chamber cpl. (3) (clean or new) into the electronics unit (5) until the mechanical stop is reached.



Pins aligned straight.

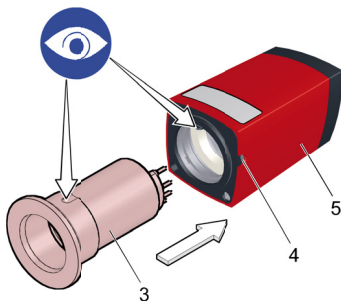

- ⑦ Fasten the measuring chamber (3) by means of the hexagon socket set screw (4).


### 6.2.3 Replacing Measuring Chamber

#### Precondition

Troubleshooting (measuring chamber) performed (→ 31).





- 1 Set the calibration value of the spare sensor with the <CAL> switch on the electronics unit (5).

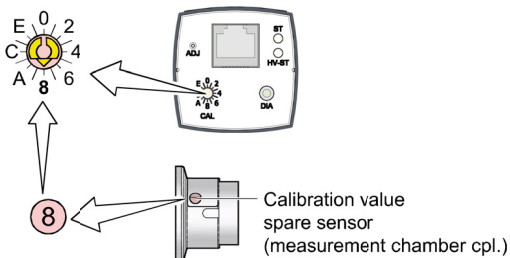


- 2 Carefully slide the measuring chamber cpl. (3) into the electronics unit (5) until the mechanical stop is reached.



Pins aligned straight.

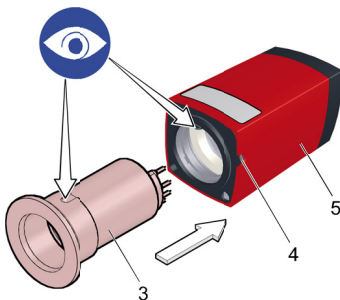

- 3 Fasten the measuring chamber (3) by means of the hexagon socket set screw (4).
- 4 Perform an ATM and HV adjustment of the Pirani measuring circuit via the <ADJ> button (→  28).
- 5 We recommend to perform a leak test (leak rate  $<1 \times 10^{-9}$  mbar l/s) and a function test of the gauge on the leak detector.

**WARNING**

WARNING: electric arcing

Helium may cause electric arcing with detrimental effects on the electronics of the product.

Before performing any tightness tests put the product out of operation and remove the electronics unit.

## 6.3 Troubleshooting



In case of an error, it may be helpful to just turn off the mains supply and turn it on again after 5 s.



Problem	LED <ST>	LED <HV-ST>	Possible cause	Correction
No voltage at signal output.	off	off	No supply voltage.	Turn on power supply.
Measuring signal unstable.	lid solid green	lid solid green	Gauge contaminated.	Replace ionization chamber or measuring chamber cpl (→ 33, 35).
Voltage at signal output does not drop under <4.82 V.	lid solid yellow	blinking green	Gas discharge has not ignited.	Wait, until the gas discharge has ignited (=5 minutes at a pressure of $10^{-9}$ mbar).
Voltage at signal output continually > 5.6 V.	lid solid green	off	Pirani zero point shift.	Perform a HV adjustment via button (→ 29).
Voltage at signal output continually > 9.5 V.	lid solid red	off	Pirani defective.	Replace the measuring chamber cpl. (→ 35).
	blinking red	off	EEPROM error.	Switch the gauge off and on again after 5 s. Replace the gauge.
Signal continually at approx. $5 \times 10^{-4}$ mbar.	lid solid green	lid solid green	Measuring chamber severely contaminated.	Replace the measuring chamber cpl. (→ 35).



## 7 Returning the Product



### WARNING

**WARNING:** forwarding contaminated products  
Contaminated products (e.g. radioactive, toxic, caustic or microbiological hazard) can be detrimental to health and environment.

Products returned to Pfeiffer Vacuum should preferably be free of harmful substances. Adhere to the forwarding regulations of all involved countries and forwarding companies and enclose a duly completed declaration of contamination<sup>\*)</sup>.

<sup>\*)</sup> Form under [www.pfeiffer-vacuum.com](http://www.pfeiffer-vacuum.com)

Products that are not clearly declared as "free of harmful substances" are decontaminated at the expense of the customer. Products not accompanied by a duly completed declaration of contamination are returned to the sender at his own expense.



## 8 Disposal



### DANGER

**DANGER:** contaminated parts

Contaminated parts can be detrimental to health and environment.

Before beginning to work, find out whether any parts are contaminated. Adhere to the relevant regulations and take the necessary precautions when handling contaminated parts.



### WARNING



**WARNING:** substances detrimental to the environment

Products or parts thereof (mechanical and electric components, operating fluids etc.) can be detrimental to the environment.

Dispose of such substances in accordance with the relevant local regulations.

### Separating the components

After disassembling the product, separate its components according to the following criteria:

- Contaminated components

Contaminated components (radioactive, toxic, caustic or biological hazard etc.) must be decontaminated in accordance with the relevant national regulations, separated according to their materials, and disposed of.

- Other components

Such components must be separated according to their materials and recycled.





## 9 Options

	Ordering No.
Seal with centering ring and fine filter 4 $\mu\text{m}$ , DN 25 ISO-KF (stainless steel /FPM)	PT 120 036 -T
Seal with centering ring and fine filter 20 $\mu\text{m}$ , DN 25 ISO-KF (stainless steel /FPM)	PF 117 225 -T

## 10 Accessories

	Ordering No.
Mounting / removing tool for ignition aid	PT 120 316 -T
Sensor cable FCC 68, 3 m	PT 448 450 -T



## 11 Spare Parts

When ordering spare parts, always indicate:

- all information on the product nameplate
- description and ordering number

### 11.1 Ignition Aid

	Ordering No.
Ignition aid (set of 10 pieces)	BN 845 995 -T


### 11.2 Ionization chamber

	Ordering No.
Ionization chamber stainless steel	PT 120 312 -T



### 11.3 Measuring Chamber Cpl. (Spare Sensor)

The measuring chamber cpl. is pre-assembled.

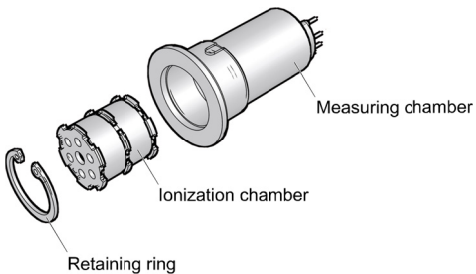

			Ordering No.
PTR 91	PT T03 148 310	DN 25 ISO-KF	PT 120 302 -T
	PT T03 158 310	DN 40 ISO-KF	PT 120 306 -T
	PT T03 358 310	DN 40 CF-F	PT 120 310 -T



## ETL Certification

RECOGNIZED  
COMPONENT



**Intertek**  
3103457

ETL LISTED

The product PTR 91

- conforms to the UL Standard UL 61010-1
- is certified to the CAN/CSA Standard C22.2 No. 61010-1-12



## EU Declaration of Conformity



We, Pfeiffer Vacuum, hereby declare that the equipment mentioned below complies with the provisions of the Directive relating to electromagnetic compatibility 2014/30/EU and the Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment 2011/65/EU.

### FullRange<sup>®</sup> Gauge

PTR 91

#### Standards

Harmonized and international / national standards and specifications:

- EN 61000-6-2:2005 (EMC: generic immunity standard)
- EN 61000-6-3:2007 + A1:2011 (EMC: generic emission standard)
- EN 61010-1:2010 (Safety requirements for electrical equipment for measurement, control and laboratory use)
- EN 61326-1:2013 (EMC requirements for electrical equipment for measurement, control and laboratory use)

#### Manufacturer / Signatures

Pfeiffer Vacuum GmbH, Berliner Straße 43, D-35614 Asslar

12 April 2016

Dr. Ulrich von Hülsen  
Geschäftsführer



## Notes



## Notes



## VACUUM SOLUTIONS FROM A SINGLE SOURCE

Pfeiffer Vacuum stands for innovative and custom vacuum solutions worldwide, technological perfection, competent advice and reliable service.

## COMPLETE RANGE OF PRODUCTS

From a single component to complex systems:

We are the only supplier of vacuum technology that provides a complete product portfolio.

## COMPETENCE IN THEORY AND PRACTICE

Benefit from our know-how and our portfolio of training opportunities!

We can support you with your plant layout and provide first-class on-site-service worldwide.

Are you looking for a  
perfect vacuum solution?  
Please contact us

Pfeiffer Vacuum GmbH  
Headquarters • Germany  
Tel.: +49 6441 802-0  
info@pfeiffer-vacuum.de

[www.pfeiffer-vacuum.com](http://www.pfeiffer-vacuum.com)

**PFEIFFER**  **VACUUM**



bg5041ben/ b



聚天真空  
HT VACUUM